

1 This article has been accepted for publication in Infection Ecology & Epidemiology published by Taylor &  
2 Francis

## 3 4 **Evaluation of a COVID-19 IgM and IgG rapid test; an efficient tool for** 5 **assessment of past exposure to SARS-CoV-2**

6  
7 Tove Hoffman<sup>1</sup>, Karolina Nissen<sup>2</sup>, Janina Krambrich<sup>1</sup>, Bengt Rönnberg<sup>1,3</sup>, Dario Akaberi<sup>1</sup>,  
8 Mouna Esmaeilzadeh<sup>1</sup>, Erik Salaneck<sup>1,2</sup>, Johanna Lindahl<sup>1,4,5</sup>, Åke Lundkvist<sup>1</sup>

9 <sup>1</sup> Department of Medical Biochemistry and Microbiology, Zoonosis Science Center (ZSC), Uppsala University,  
10 Uppsala, Sweden

11 <sup>2</sup> Department of Medical Sciences, Infectious diseases, Uppsala University, Uppsala, Sweden

12 <sup>3</sup> Laboratory of Clinical Microbiology, Uppsala University Hospital, Uppsala, Sweden

13 <sup>4</sup>Department of Clinical Sciences, Swedish University of Agricultural Sciences, Uppsala, Sweden

14 <sup>5</sup>Department of Biosciences, International Livestock Research Institute, Hanoi, Vietnam

### 15 16 **Corresponding author:**

17 Åke Lundkvist, PhD, Prof.

18 ake.lundkvist@imbim.uu.se

### 19 20 **Abstract**

21 COVID-19 is the most rapidly growing pandemic in modern time, and the need for  
22 serological testing is most urgent. Although the diagnostics of acute patients by RT-PCR is  
23 both efficient and specific, we are also crucially in need of serological tools for investigating  
24 antibody responses and assessing individual and potential herd immunity. We evaluated a  
25 commercially available test developed for rapid (within 15 minutes) detection of SARS-CoV-  
26 2-specific IgM and IgG by 29 PCR-confirmed COVID-19 cases and 124 negative controls.  
27 The results revealed a sensitivity of 69.0 % and 93.1 % for IgM and IgG, respectively, based  
28 solely on PCR-positivity due to the absence of a serological gold standard. The assay  
29 specificities were shown to be 100 % for IgM and 99.2 % for IgG. This indicates that the test  
30 is suitable for assessing previous virus exposure, although negative results may be unreliable  
31 during the first weeks after infection. More detailed studies on antibody responses during and  
32 post infection are urgently needed.

33  
34 **Keywords:** COVID-19, SARS-CoV-2, rapid test, IgM, IgG, diagnostics

35

36

37

## 38 **Background**

39 In late 2019, a cluster of cases of viral pneumonia of unknown aetiology was reported in  
40 Wuhan, Hubei Province, China. This new viral pneumonia, COVID-19 (Coronavirus Disease  
41 2019), caused by the novel SARS-CoV-2 (Severe Acute Respiratory Syndrome Coronavirus-  
42 2), spread rapidly and developed into a global pandemic within three months from its initial  
43 detection (1–3). Among other symptoms those of COVID-19 often include fever and dry  
44 cough, which resemble respiratory illnesses caused by other viruses or bacteria (4–7). Due to  
45 the overlapping manifestations, clinical diagnosis becomes problematic, especially during  
46 seasonal flu (8), why confirmation of COVID-19 depends on the detection of SARS-CoV-2  
47 nucleic acid by reverse-transcriptase polymerase chain reaction (RT-PCR).

48 More than 1.26 million cases of COVID-19 in > 200 countries and territories, with more than  
49 66.000 human deaths, have been reported (9, April 5, 2020). Due to the limited testing in  
50 many geographical regions, it is clear that the total number of actual COVID-19 cases is much  
51 higher than the number of confirmed ones. In most of the confirmed COVID-19 cases, the  
52 patients are symptomatic showing fever, dry cough, and pneumonia, but also more atypical  
53 symptoms such as gastrointestinal manifestations as well as anosmia and ageusia. However,  
54 the virus has been detected in completely asymptomatic individuals, e.g. in a recent study  
55 from Italy, showing that 44 % of the laboratory-confirmed cases lacked symptoms (10). The  
56 knowledge concerning the actual number of asymptomatic vs. symptomatic infections is still  
57 limited. The same is true for the potentially growing herd immunity, where almost no data is  
58 available to date.

59 In the present study, we evaluated a commercially available assay, the COVID-  
60 19 IgG/IgM Rapid Test Cassette (Zhejiang Orient Gene Biotech Co Ltd, Huzhou, Zhejiang,  
61 China), developed for detection of SARS-CoV-2-specific antibodies.

62

63

## 64 **Material and Methods**

### 65 Serum samples

66 Capillary blood samples or serum from 29 PCR-confirmed COVID-19 patients or  
67 convalescents, and capillary blood samples from 24 healthy volunteers, without any known  
68 history of SARS-CoV-2 infection/COVID-19, were included in the study. Anonymous blood

69 donor sera from healthy adults (n=80) and 20 serum samples from babies (6-12 months) from  
70 the Uppsala Academic Hospital were used as negative controls. Clinical samples that had  
71 been deposited in Uppsala Biobank were anonymized and used in accordance with local  
72 ethical guidelines. They were all used with informed consent according to the Swedish  
73 Biobank law, which allows anonymized diagnostic patient samples to be used for purposes  
74 similar to those of the original sampling. The 29 samples from COVID-19 confirmed  
75 individuals, as well as the 100 negative controls and the 24 healthy volunteers were all from  
76 unique individuals. All samples were analyzed anonymously.

77

#### 78 COVID-19 IgG/IgM rapid test

79 The test was run according to the manufacturers instructions (COVID-19 IgG/IgM Rapid Test  
80 Cassette (whole blood/serum/plasma), Product/Model: GCCOV-402a, Lot: 2003242, Zhejiang  
81 Orient Gene Biotech Co Ltd, Huzhou, Zhejiang, China) (11). Briefly, 5 µl of serum or one  
82 drop of capillary blood were added to the test slide, followed by 80 µl of the buffer provided  
83 in the kit. The results were read after 10 min (max 15 min), by the naked eye. Only tests in  
84 which the control line changed its color were regarded as valid (3 out of 153 tests did not  
85 work). If a line was observed for IgM and/or IgG, the test was considered positive. The  
86 intensity of the color was not judged.

87

88

### 89 **Results**

#### 90 IgM and IgG reactivities in negative control samples

91 None of the 80 negative sera from healthy blood donors tested IgM positive in the assay,  
92 while one tested IgG positive (1/80, 1.25 %, 95 % confidence level: 0.03-6.77 %) (Tables 1  
93 and 2). The single IgG-positive sample was re-analyzed and remained IgG positive in the  
94 second test. None of the 20 serum samples from the 6-12 months old babies tested positive for  
95 either IgM or IgG.

96

#### 97 IgM- and IgG-reactivities in healthy volunteers


98 None of the 24 healthy volunteers, without any known history of SARS-CoV-2  
99 infection/COVID-19, tested positive for IgM or IgG.

100

#### 101 IgM- and IgG-reactivities in PCR-confirmed COVID-19 patients

102 Altogether 20 of 29 (69 %) samples from PCR-confirmed COVID-19 patients tested IgM  
 103 positive and 27 tested (93.1 %) IgG positive (Tables 1 and 2). When the patients were  
 104 grouped into two groups depending on the time between onset of disease and testing, seven  
 105 out of ten patients in the first group (9-17 days) and 13/19 patients in the second group (18-29  
 106 days) tested IgM positive. Nine out of ten patients in the first group (9-17 days) and 18/19  
 107 patients in the second group (18-29 days) tested IgG positive (Figure 1). There was no  
 108 statistical difference between the two groups for neither IgM or IgG seropositivity. All  
 109 samples that were IgM positive were also IgG positive.

110

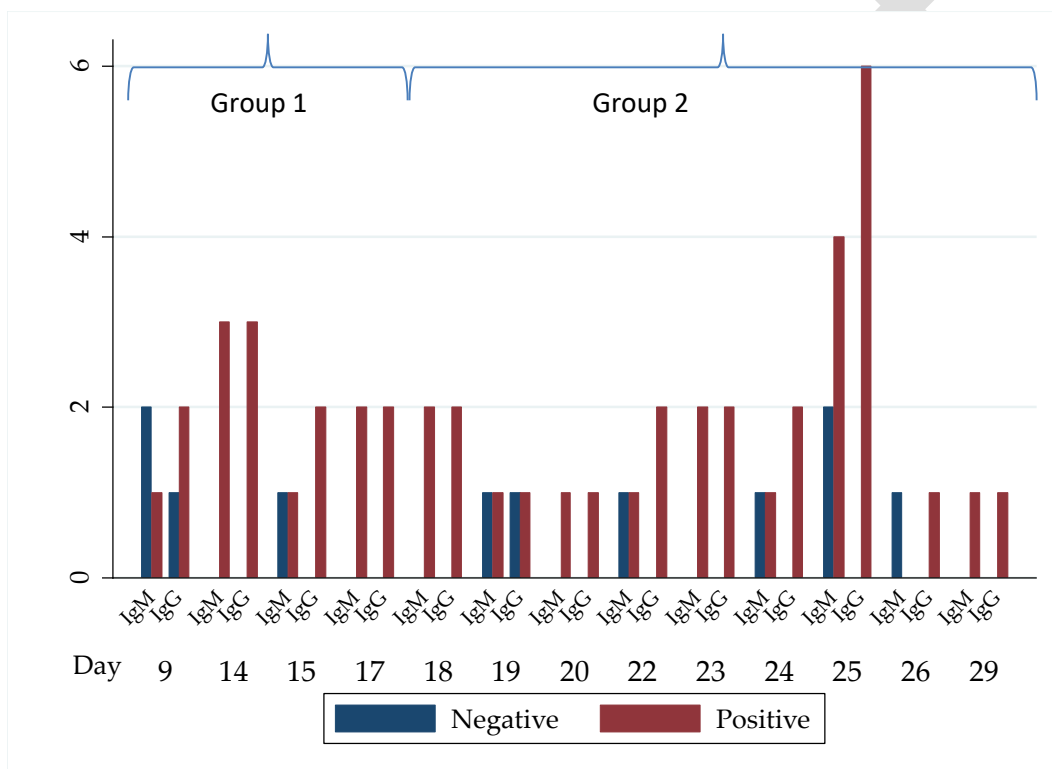

111

112 Figure 1. Number of PCR-positive cases positive or negative for IgM or IgG based on number  
 113 of days after onset of COVID-19 symptoms.

114

115 Assay sensitivity, specificity and accuracy

116 Based on the results described above and summarized in Tables 1 and 2, the assay showed a  
 117 sensitivity of 69.0 % (20/29) and 93.1 % (27/29) for IgM and IgG, respectively. The assay  
 118 showed an overall specificity of 100 % (124/124) and 99.2 % (123/124, 1 false positive) for  
 119 IgM and IgG, respectively.

120 Using PCR-positive cases as true positives, the accuracy of the test was 94.1 %  
 121 (144/153) and 98.0 % (150/153) for IgM and IgG, respectively. The positive and negative  
 122 predictive values (the likelihood of being a case given a positive test result, and the likelihood  
 123 of being healthy given a negative test result) for IgM were 100 % (20/20) and 93.2 %  
 124 (124/133), respectively. For IgG, the corresponding values were 96.4 % (27/28) and 98.4 %  
 125 (123/125).

126

127 Table 1. Comparisons of IgM results for 29 PCR-positive COVID-19 cases and 124 healthy individuals.

|              | Cases | Healthy | Total |
|--------------|-------|---------|-------|
| IgM positive | 20    | 0       | 20    |
| IgM negative | 9     | 124     | 133   |
| Total        | 29    | 124     | 153   |

128

129

130

131 Table 2. Comparisons of IgG results for 29 PCR-positive COVID-19 cases and 124 healthy individuals.

|              | Cases | Healthy | Total |
|--------------|-------|---------|-------|
| IgG positive | 27    | 1       | 28    |
| IgG negative | 2     | 123     | 125   |
| Total        | 29    | 124     | 153   |

132

133

### 134 Discussion

135 In this study we evaluated a commercial rapid test for detection of SARS-CoV-2-specific IgM  
 136 and IgG. For the evaluation, samples from COVID-19 cases, obtained during disease or  
 137 convalescence and previously confirmed by PCR, were used as “true positives”. This means  
 138 that in the PCR positive cases for which antibodies may not yet had time to develop, or in  
 139 potential cases with immune defects, it is possible that the negative IgM or IgG results were  
 140 in fact true negatives. If this was the case for one or more of the included patients, the actual  
 141 sensitivities should be higher, i.e. when evaluated only on samples known to contain  
 142 detectable levels of SARS-CoV-2-specific IgM and/or IgG. For a more optimal evaluation of  
 143 the assay sensitivity, a gold standard for SARS-CoV-2-specific antibodies would have been  
 144 needed. This is, however, unfortunately not available to date.

145 According to the manufacturer, the specificity has been evaluated on 14 PCR-negative  
146 samples and was found to be 100% for both IgM and IgG, while the sensitivity evaluated on  
147 COVID-19 cases was calculated at 87.9 % for IgM and 97.2 % for IgG. The results by Li et  
148 al. (11) indicated an overall testing sensitivity of 88.7% and 90.6 % specificity. Our results  
149 showed a lower sensitivity for IgM, a similar sensitivity for IgG, and specificities in between  
150 the results of the two evaluations.

151 A recent study on three Chinese COVID-19 cases found that seroconversions  
152 occurred between 7 and 12 days after the onset of symptoms (12). However, larger studies on  
153 the detailed kinetics of the antibody responses (e.g. IgA, IgM, IgG, neutralizing antibodies)  
154 are now urgently needed for a better understanding of the dynamics of the immune response  
155 during COVID-19. The results of our study showed detectable IgM and IgG in some patients  
156 at day 9, while in other patients the seroconversion seems to occur later. The impact of early  
157 or late seroconversion on the case severity is not known, and must now be explored.  
158 Interestingly, there were no IgM positives that were not IgG positive. Generally, IgM is  
159 produced first, and later there is a switch towards IgG production (13), but studies on SARS-  
160 CoV suggest that IgM and IgG often develop around the same time (14, 15). Our results are in  
161 line with this (Figure 1), but more detailed studies on long-term sequential samples from  
162 patients are now needed. It may be worth looking into whether this is a problem with the test,  
163 or a constant finding within the immune response to SARS-CoV-2.

164 There were no false IgM positive samples, indicating a very high specificity of  
165 the test. One false positive IgG result was observed for one healthy adult blood donor. This  
166 sample was re-tested and the result was consistent, indicating a cross-reaction to another  
167 coronavirus. Serological cross-reactions have earlier been observed between SARS-CoV and  
168 SARS-CoV-2 (16). There are other human coronaviruses (NL63, OC43, 229E, and HKU1)  
169 that are globally endemic or epidemic (17), and it may be possible that this reaction  
170 represented a cross-reaction due to a previous infection with one of those. Human CoV NL63  
171 has been shown to use the same receptor, angiotensin-converting enzyme 2 (ACE2), as  
172 SARS-CoV and SARS-CoV-2 (18), which may indicate potential cross-reactive epitopes.  
173 How common the CoVs are as causative agents for “common colds” is not known in detail,  
174 but there has been estimates that up to 20 % of cases could be caused by CoVs (19).

175 The specificity and sensitivity for IgG detection of the rapid test evaluated here  
176 is well in line with those of a recently reported enzyme-linked immunosorbent assay (ELISA),  
177 which had a specificity and a sensitivity of 97.5 % (20).

178                   While this study showed a satisfactory performance of the rapid test, it is limited  
179 by being compared only to clinical cases and PCR-positivity, and as a next step, it is  
180 necessary to compare this assay to other serological tests. In contrast to Li et al. (11), we  
181 found less indications for using this test for clinical diagnosis. Nevertheless, it might  
182 contribute to detecting potential asymptomatic infections as well as getting a notion of the  
183 magnitude of the spread in different geographical areas, which might be a key to taking the  
184 appropriate decisions and policies forward. The high negative predictive value indicates that  
185 the rapid test will be useful for detecting past infections and possible immunity, which may be  
186 crucial for restoring social functions after lockdown.

187

### 188 **Conflict of interest**

189 The authors declare no conflicts of interest.

190

### 191 **Acknowledgements**

192 The rapid tests that have enabled this study were donated to us by the Swedish company  
193 Noviral AB (organization number: 559175-7942).

194

### 195 **References**

- 196 1. Guarner J. Three Emerging Coronaviruses in Two DecadesThe Story of SARS, MERS,  
197 and Now COVID-19. *Am J Clin Pathol.* 2020 Mar 9;153(4):420–1.
- 198 2. De Wit E, Van Doremalen N, Falzarano D, Munster VJ. SARS and MERS: Recent  
199 insights into emerging coronaviruses [Internet]. *Nature Reviews Microbiology* Nature  
200 Publishing Group; Aug 1, 2016 p. 523–34. Available from: [www.nature.com/nrmicro](http://www.nature.com/nrmicro)
- 201 3. Hilgenfeld R, Peiris M. From SARS to MERS: 10 years of research on highly  
202 pathogenic human coronaviruses. Vol. 100, *Antiviral Research.* Elsevier; 2013. p. 286–  
203 95.
- 204 4. Wang D, Hu B, Hu C, Zhu F, Liu X, Zhang J, et al. Clinical Characteristics of 138  
205 Hospitalized Patients with 2019 Novel Coronavirus-Infected Pneumonia in Wuhan,  
206 China. *JAMA - J Am Med Assoc.* 2020;
- 207 5. Huang C, Wang Y, Li X, Ren L, Zhao J, Hu Y, et al. Clinical features of patients  
208 infected with 2019 novel coronavirus in Wuhan, China. *Lancet.* 2020 Feb  
209 15;395(10223):497–506.
- 210 6. Wu Z, McGoogan JM. Characteristics of and Important Lessons from the Coronavirus  
211 Disease 2019 (COVID-19) Outbreak in China: Summary of a Report of 72314 Cases

- 212 from the Chinese Center for Disease Control and Prevention. *JAMA - J Am Med*  
213 *Assoc.* 2020;
- 214 7. Li Q, Guan X, Wu P, Wang X, Zhou L, Tong Y, et al. Early Transmission Dynamics in  
215 Wuhan, China, of Novel Coronavirus–Infected Pneumonia. *N Engl J Med.* 2020 Jan  
216 29;
- 217 8. Wu X, Cai Y, Huang X, Yu X, Zhao L, Wang F, et al. Co-infection with SARS-CoV-2  
218 and Influenza A Virus in Patient with Pneumonia, China. *Emerg Infect Dis.* 2020  
219 Jun;26(6).
- 220 9. Worldometer. Worldometer, Coronavirus [Internet]. 2020 [cited 2020, April 4].  
221 Available from: <https://www.worldometers.info/coronavirus/>
- 222 10. ECDC. Novel coronavirus disease 2019 (COVID-19) pandemic: increased  
223 transmission in the EU/EEA and the UK – sixth update [Internet]. Stockholm, Sweden;  
224 2020. Available from: [https://www.ecdc.europa.eu/sites/default/files/documents/RRA-](https://www.ecdc.europa.eu/sites/default/files/documents/RRA-sixth-update-Outbreak-of-novel-coronavirus-disease-2019-COVID-19.pdf)  
225 [sixth-update-Outbreak-of-novel-coronavirus-disease-2019-COVID-19.pdf](https://www.ecdc.europa.eu/sites/default/files/documents/RRA-sixth-update-Outbreak-of-novel-coronavirus-disease-2019-COVID-19.pdf)
- 226 11. Li Z, Yi Y, Luo X, Xiong N, Liu Y, Li S, et al. Development and Clinical Application  
227 of A Rapid IgM-IgG Combined Antibody Test for SARS-CoV-2 Infection Diagnosis. *J*  
228 *Med Virol* [Internet]. 2020 Feb 27 [cited 2020 Apr 4];jmv.25727. Available from:  
229 <https://onlinelibrary.wiley.com/doi/abs/10.1002/jmv.25727>
- 230 12. Zhang J, Liu J, Li N, Liu Y, Ye R, Qin X, et al. Serological detection of 2019-nCoV  
231 respond to the epidemic: A useful complement to nucleic acid testing. *medRxiv.* 2020  
232 Mar 10;2020.03.04.20030916.
- 233 13. Gunther N, Hoffmann GW. Qualitative dynamics of a network model of regulation of  
234 the immune system: A rationale for the IgM to IgG switch. *J Theor Biol.* 1982 Feb  
235 21;94(4):815–55.
- 236 14. Li G, Chen X, Xu A. Profile of specific antibodies to the SARS-associated coronavirus.  
237 Vol. 349, *New England Journal of Medicine.* 2003. p. 508–9.
- 238 15. Hsueh PR, Huang LM, Chen PJ, Kao CL, Yang PC. Chronological evolution of IgM,  
239 IgA, IgG and neutralisation antibodies after infection with SARS-associated  
240 coronavirus. *Clin Microbiol Infect.* 2004 Dec 1;10(12):1062–6.
- 241 16. Wan WY, Lim SH, Seng EH. Cross-reaction of sera from COVID-19 patients with  
242 SARS-CoV assays. *medRxiv* [Internet]. 2020 Mar 23 [cited 2020 Apr  
243 1];2020.03.17.20034454. Available from:  
244 <https://www.medrxiv.org/content/10.1101/2020.03.17.20034454v1>
- 245 17. Paules CI, Marston HD, Fauci AS. Coronavirus Infections-More Than Just the



- 246 Common Cold. Vol. 323, JAMA - Journal of the American Medical Association.  
247 American Medical Association; 2020. p. 707–8.
- 248 18. Hofmann H, Pyrc K, Van Der Hoek L, Geier M, Berkhout B, Pöhlmann S. Human  
249 coronavirus NL63 employs the severe acute respiratory syndrome coronavirus receptor  
250 for cellular entry. *Proc Natl Acad Sci U S A*. 2005 May 31;102(22):7988–93.
- 251 19. Bende M, Barrow I, Heptonstall J, Higgins PG, Al-Nakib W, Tyrrell DAJ, et al.  
252 Changes in human nasal mucosa during experimental coronavirus common colds. *Acta*  
253 *Otolaryngol*. 1989;107(3–4):262–9.
- 254 20. Zhao R, Li M, Song H, Chen J, Ren W, Feng Y, et al. Serological diagnostic kit of  
255 SARS-CoV-2 antibodies using CHO-expressed full-length SARS-CoV-2 S1 proteins.  
256 medRxiv. 2020 Mar 27;2020.03.26.20042184.  
257

Preprint